

LA-UR -81-1989

TITLE: IN-LINE MEASUREMENT OF PLUTONIUM AND AMERICIUM IN MIXED SOLUTIONS

AUTHOR(S): T. K. Li

MASTER

SUBMITTED TO: 22nd Annual Meeting
Institute of Nuclear Materials Management
San Francisco, California
July 13-15, 1981



University of California

By acceptance of this article, the publisher recognizes that the U.S. Government retains a nonexclusive, royalty-free license to publish or reproduce the published form of this contribution, or to allow others to do so, for U.S. Government purposes.

The Los Alamos Scientific Laboratory requests that the publisher identify this article as work performed under the auspices of the U.S. Department of Energy.



LOS ALAMOS SCIENTIFIC LABORATORY

Post Office Box 1663 Los Alamos, New Mexico 87545

An Affirmative Action/Equal Opportunity Employer



286

IN-LINE MEASUREMENT OF PLUTONIUM AND AMERICIUM IN MIXED SOLUTIONS*

T. K. Li
University of California
Los Alamos National Laboratory
Los Alamos, NM 87545

ABSTRACT

A solution assay instrument (SAI) has been developed at the Los Alamos National Laboratory and installed in the plutonium purification and americium recovery process area in the Los Alamos Plutonium Processing Facility. The instrument is designed for accurate, timely, and simultaneous nondestructive analysis of plutonium and americium in process solutions that have a wide range of concentrations and Am/Pu ratios. For a 25-ml sample, the assay precision is <1%, both for plutonium and for americium having concentrations >5 g/L within a 2000-s count time.

INTRODUCTION

During the past several years, the Plutonium Processing Facility at the Los Alamos National Laboratory has prepared ceramic-grade plutonium dioxide in production quantities by purifying impure plutonium metal to plutonium oxide.¹ Large quantities of americium and other impurities are removed from the plutonium as peroxide filtrates in this process. Because of the increasing demand for the use of americium in oil-well logging instruments and other uses, routine operations to recover the americium have been developed and implemented.² Figure 1 shows partial flow diagrams for a plutonium purification process based on selective precipitation and an americium recovery and purification process based on ion exchange and oxalate precipitation.

The solutions generated from the plutonium purification and americium recovery processes have a wide range of total (plutonium and americium) concentrations and Am/Pu ratios: for solutions generated from the plutonium purification process, the total concentrations range from 0.1 to 500 g/L and the Am/Pu ratios vary from a few parts per million to 10; for solutions generated from the americium recovery process, the total concentrations range from 0.1 to 50 g/L and the Am/Pu ratios vary from 0.5 to 100.

It is important to both special nuclear material control and process control to determine

*This work was performed under the auspices of the US Department of Energy.

the plutonium and americium content of these solutions accurately and rapidly. The assay procedure needs to be as simple as possible for routine operation by process technicians. An in-line solution assay instrument (SAI) that satisfies these criteria has been designed at Los Alamos and installed in the plutonium purification and americium recovery process area in the Los Alamos Plutonium Processing Facility. Solution types, with total concentration and A/Pu ratios, are shown at the SAI measurement points in Fig. 1.

MEASUREMENT METHOD

The SAI is based upon high-resolution gamma-ray measurements. Because the plutonium in the purification process is of known isotopic composition, the total plutonium concentration of the solutions can be determined by using the 413.7-keV gamma rays from ²³⁹Pu. The americium concentration is determined by a weighted average based on the measured intensities of the 376.6-keV (after removal of the contribution from ²³⁹Pu at 375 keV) and 419-keV gamma rays from ²⁴¹Am. The reason for not using high-intensity low-energy gamma rays (for example, 125 keV, 129 keV) is because the correction factors and uncertainties become very large; the transmission of low-energy gamma rays decreases dramatically as the total concentration increases up to 200 g/L. Furthermore, as the ²⁴¹Am/²³⁹Pu ratios and/or ²³⁷U/²³⁹Pu ratios in the solutions become very high, the Compton continuum from the intense 208-keV gamma ray makes the lower energy unusable. To maximize the SAI's sensitivity and precision at both low and high concentrations for such high ratios, a 0.76-mm-thick tungsten filter was installed in front of the detector. The filter reduces the lower energy portion of the gamma-ray spectrum and provides adequate reduction of the 416-keV sum peak that results from pileup of the 208-keV gamma rays and interferes with the 413.7-keV ²³⁹Pu peak. The transmission correction is made by counting gamma rays emitted from an external transmission source (a 20-g nickel-plated plutonium metal disk) through the sample. Corrections for rate-related counting losses as a result of dead time and pile-up are made by counting the 88-keV gamma rays

emitted from a ^{109}Cd source attached directly to the detector housing.

The gamma-ray net peak areas are calculated by using a straight-line background subtraction method. Both the 413.7- and 419-keV gamma rays are clean single peaks, while the 376.6-keV gamma rays are part of an unresolved doublet that includes the contribution from ^{239}Pu at 375 keV. The americium content determined from the unresolved doublet can be expressed as follows:

$$\text{Am (g)} = \frac{I}{I(376.6)} \left[\frac{R}{F} - \frac{I(375)}{I} \times {}^{239}\text{Pu (g)} \right]$$

where

$I(375)$, $I(376.6)$ = specific activity of 375-, 376.6-keV gamma rays, respectively, (in $\gamma/\text{g/s}$).

$$I = I(375) + I(376.6).$$

R = count rate of (375 + 376.6) unresolved peak (in counts/s) with the corrections of transmission and rate-related counting losses,

${}^{239}\text{Pu}$ = ${}^{239}\text{Pu}$ content (in g) in the sample as determined by the intensity of 413.7 keV,

$$K = \text{calibration constant (in counts/G/s),}$$

and

$$G = \frac{I(375)}{I} \times {}^{239}\text{Pu(g)} + \frac{I(376.6)}{I} \times {}^{241}\text{Am(g)}.$$

The SAI hardware, software, and assay procedure have been described elsewhere.³ Briefly, the SAI consists of a sample chamber, a germanium detector and associated electronics, a NOVA 2 (28K of 16-bit memory) minicomputer-based multi-channel analyzer with a digitally stabilized 4K analog-to-digital converter, a dual magnetic-tape cassette unit, and a terminal. The sample chamber houses a polystyrene sample bottle and a rotating tungsten shutter. The sample bottle is a right circular cylinder (10 cm² by 4 cm) with a maximum solution volume of 40 mL. For routine assays, 25-mL solution samples are drawn through clean calibrated automatic pipettes by process technicians. The shutter is located above the sample bottle and is pneumatically operated under computer control; the transmission source is centered on one side of the shutter. The germanium detector, which has a resolution of 1.55 keV at 413.7 keV, is located outside the glovebox, directly under the sample bottle. No modifications were necessary to the 4.75-mm-thick stainless steel glovebox floor.

An automatic data-acquisition-and-analysis program written in interactive BASIC language gives simple instructions for the assay procedure and asks the operator to respond to displayed

questions by entering numerical codes at the terminal.

The assay procedure includes a background run, a transmission-source run, a transmission-source-plus-sample run, and a sample-only run. The background run and the transmission-source run are required once a day; the data are stored in the computer. The transmission-source-plus-sample run and the sample-only run are performed for each sample; the system automatically combines the resulting data with the stored background and transmission-source data for calculating the final assay results. The data collection times for the concentrated solutions were 1000-s (500-s each for the transmission-plus-sample run and for the sample-only run). For low-concentration solutions, the data collection times were 2000-s (100-s for the transmission-plus-sample run and 1900-s for the sample-only run).

RESULTS AND DISCUSSION

The instrument was calibrated with solution standards prepared by the Analytical Chemistry Laboratory at Los Alamos. Six plutonium standards, having concentrations ranging from 0.45 to 261 g Pu/L, were used for the original plutonium calibration. The typical precision of the plutonium assay³ was <0.75% for concentrations >30 g Pu/L within a 1000-s count time and ~4% at 0.5 g Pu/L within a 2000-s count time. Four americium standards, having concentrations ranging from 0.1 to 4.5 g Am/L, were used for americium calibration. The precision of the americium analysis was <1% for concentrations >4.5 g Am/L and ~4% at 0.3 g Am/L within a 2000-s count time.

The performance of the SAI in assaying plutonium process solutions³ has been evaluated by comparing results from its analyses with results from chemical analyses (photometric titration). The results agreed very well for plutonium solutions that were free of particulate matter.

The SAI accuracy for simultaneous analysis of americium and plutonium in mixed solutions from process samples is tested by comparing the SAI results with those of radioanalysis. Radioanalysis, which is routinely used for analyzing process samples, determines (1) plutonium content by alpha counting after the plutonium is extracted with 2-thenoyl trifluoroacetone and (2) americium content⁴ by integral counting gamma activity above 32 keV. The routine accuracy of the radioanalysis is ~1 to 5% for americium and ~5 to 10% for plutonium. Preliminary results for 15 process samples are summarized in Table I. The radioanalysis results and their associated uncertainties are the means and mean deviations of two measurements, respectively. Although the plutonium concentrations were relatively low (<1.2 g Pu/L) and Am/Pu ratios were relatively high (from 0.6 to 34.9), the average relative difference between the SAI and radioanalysis results was 0.21%, which indicates that there is no significant bias between them. However, an

TABLE I
COMPARISON OF SAI RESULTS WITH RADIOANALYSIS RESULTS FOR SIMULTANEOUS
AMERICIUM AND PLUTONIUM MEASUREMENTS

Sample No.	Am Concentration (g/L)			Pu Concentration (g/L)			Am/Pu ^c
	RAD ^a	SAI	$\Delta\%$ ^b	RAD	SAI	$\Delta\%$	
1	0.90 ± 0.02	0.86 ± 0.02	-4.4	0.88 ± 0.02	0.92 ± 0.04	4.6	0.9
2	0.41	0.39 ± 0.02	-4.9	0.098 ± 0.004	0.116 ± 0.04	18.4	3.4
3	3.10 ± 0.07	3.06 ± 0.03	-1.3	0.68	0.55 ± 0.07	-4.4	4.7
4	5.15	4.87 ± 0.05	-5.4	0.97 ± 0.02	0.89 ± 0.09	-8.3	5.5
5	3.10	2.68 ± 0.03	-13.6	0.83 ± 0.04	0.90 ± 0.07	8.4	3.0
6	1.56 ± 0.06	1.54 ± 0.02	-1.3	0.068 ± 0.02	0.053 ± 0.05	-22.1	29.1
7	2.39	2.20 ± 0.03	-7.9	0.99 ± 0.04	1.14 ± 0.06	15.2	1.9
8	3.95	3.87 ± 0.04	-2.0	1.02 ± 0.05	1.03 ± 0.08	1.0	3.8
9	1.90 ± 0.07	1.85 ± 0.02	-2.6	0.057 ± 0.002	0.053 ± 0.058	-7.0	34.9
10	2.36	2.39 ± 0.04	1.3	0.67 ± 0.02	0.80 ± 0.07	19.4	3.0
11	3.81	3.73 ± 0.04	-2.1	1.15 ± 0.05	0.93 ± 0.08	-19.1	4.0
12	4.41	4.10 ± 0.04	-7.0	0.91 ± 0.04	0.70 ± 0.08	-23.1	5.9
13	3.43 ± 0.04	3.35 ± 0.04	-2.3	0.54 ± 0.02	0.535 ± 0.076	-0.9	6.3
14	3.25	3.00 ± 0.03	-7.7	0.66 ± 0.01	0.59 ± 0.07	-10.6	5.1
15	0.049	0.044 ± 0.01	-10.2	0.060 ± 0.01	0.079 ± 0.035	31.7	0.6

^aRadioanalysis results and their associated uncertainties are represented by the means and mean deviations, respectively, of two measurements. Mean deviations <1% are not listed in the table.

^b $\Delta\% = (SAI - RAD)/RAD$

^cAccording to SAI results

-5% negative bias was obtained between SAI and radioanalysis results for americium concentrations. The possible explanation for the higher radioanalysis results may be due to contribution of ²³⁷U to the 59.5-keV gamma ray, which is commonly associated with ²⁴¹Am. To obtain the best results for americium from radioanalysis, the uranium needs to be separated from the americium. Investigation is now under way to compare the radioanalysis results obtained after the uranium is removed.

ACKNOWLEDGMENT

The author wishes to thank T. Blum, D. Padella, H. Ramsey, M. Haas, and all personnel involved with the Los Alamos americium recovery process. Much of this work would be impossible without their assistance and cooperation.

REFERENCE

1. L. W. Reese, G. L. Taylor, and M. Haas, "Preparation of Ceramic Grade Plutonium Di-


oxide for the Fast Flux Test Facility," 179th American Chemical Society Meeting, Houston, Texas, March 24-30, 1980.

2. H. D. Ramsey, D. G. Clifton, S. W. Hayter, R. A. Penneman, and E. L. Christensen, "Status of ²⁴¹Am Recovery and Purification at the Los Alamos National Laboratory," Symp. on Industrial Scale-Production-Separation-Recovery of Transplutonium Elements, Second Chemical Congress of the North American Continent, Las Vegas, Nevada, August 24-30, 1980.

3. T. K. Li, "Automated In-Line Measurement of Plutonium Solutions in the FFTF Plutonium Purification Process," to be published in Nucl. Technol.

4. Joseph Bubernak, M. S. Lew, and G. W. Matlack, "Determination of Americium in Plutonium by Gamma Counting," Anal. Chem. 30, 1759 (1958).

PLUTONIUM PURIFICATION PROCESS

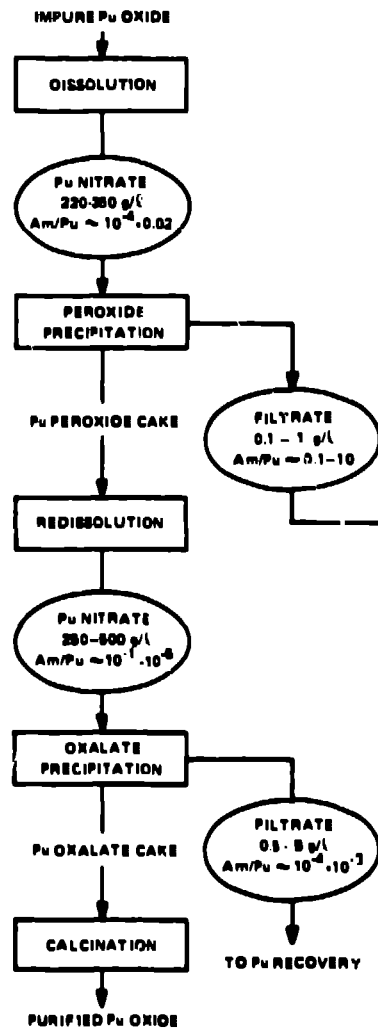

AMERICIUM PURIFICATION PROCESS

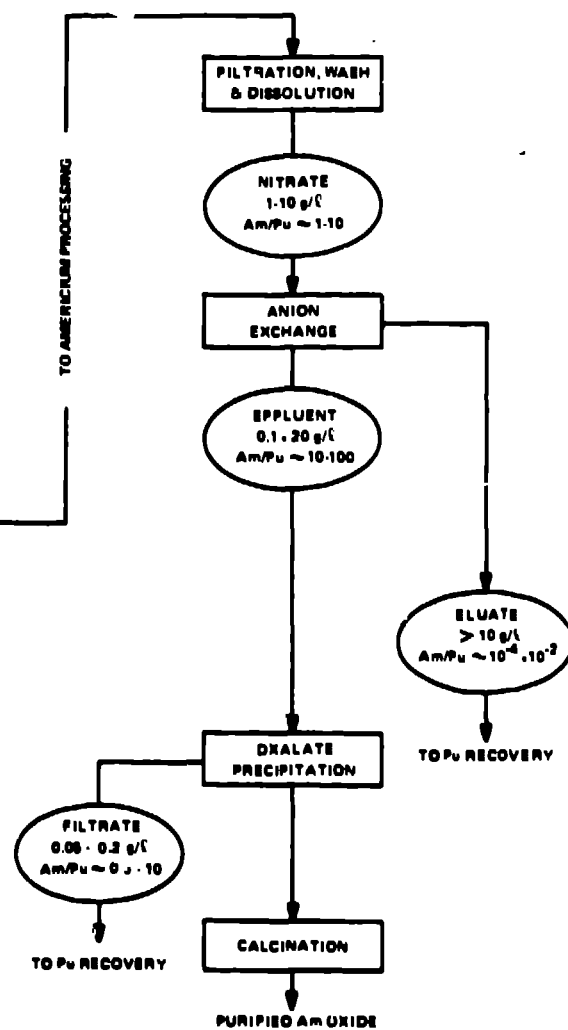


Fig. 1. Flow diagram of the plutonium purification process and the americium recovery and purification process. Solution types, with total (plutonium and americium) concentrations and Am/Pu ratios, are shown at the SAI measurement points.